




Indiana State Department of Health  
 Genomics and Newborn Screening Program  
Invalid Heelstick Results Protocol

*NOTE: For the well-being of the child, it is imperative to acquire the rescreen and without further delay, repeat the collection of specimen within five (5) business days of initial screen.*

**TAKE ACTION IN CORRECTING HEELSTICK COLLECTION TECHNIQUE TO AVOID FUTURE INVALID SCREENS DUE TO QUALITY AND OR TIMELINESS**

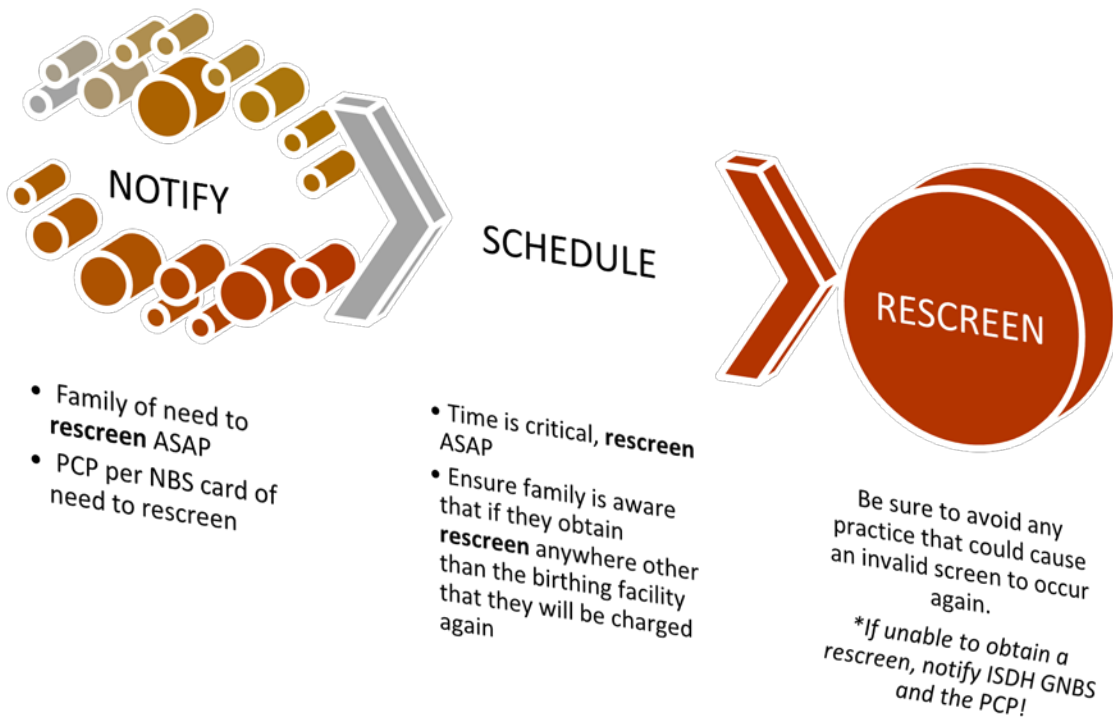


---

Please refer to any recommendations provided to you by the NBS Lab within the results. For any questions regarding lab results, please contact us at 888.815.0006